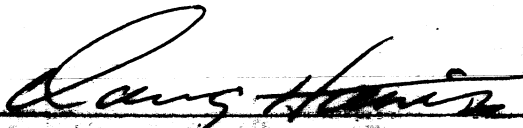


VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument


State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program


Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130115
Name	DOUG HARRIS	ID#	5530
Date	APRIL 12-09		
Agency	BRISTOL BAY POLICE DEPT.		Phone # 246-4222
Instrument Location	BRISTOL BAY POLICE DEPT. KING SALMON, ALASKA		
Alco S/N	X172961 ✓	Target Value	.082 ✓
		High Pressure	30.09
Alco Test Values			
1 st Alco	.082 ✓	2 nd Alco	.083 ✓
Signature			
	003 4/13/09		


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 19th day of May, 2009.

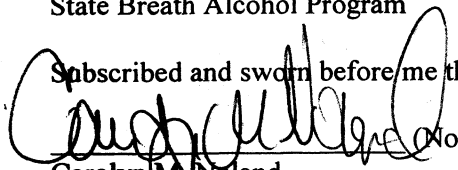
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster edm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster edm S/N 130115 ✓

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
SCIENTIFIC CRIME DETECTION LABORATORY

DATE: 04/12/2004

✓
CS
3/18/04

VERIFICATION NUMBER: 0070
SUBJECT'S LAST NAME: DOE
SUBJECT'S FIRST NAME: DOE
D.L. #: 0000000
DEPT/AGENCY: NWAD
TEST REPORT: 000000
TEST TYPE: T
ALCOHOL VALUE: 0.01 ✓
ALCOHOL S/N: 1170911 ✓

BREATH ANALYSIS

TEST INITIATED FOR 00.29 in ✓
ALCOHOL TEST 0.02 15:33
BURN TEST 0.00 15:34
INTERNAL FLOWMETER 0.0151 15:35
CHECK VALVE 0.02 ✓ 15:36
SAMPLE TEST 0.02 15:37
CHECK VALVE 0.02 ✓ 15:38
BURN TEST 0.00 ✓ 15:39
INTERNAL FLOWMETER 0.0151 ✓ 15:40
CHECK VALVE 0.02 ✓ 15:41
BURN TEST 0.00 ✓ 15:42
INTERNAL FLOWMETER 0.0151 ✓ 15:43

ALASKA DEPARTMENT OF PUBLIC SAFETY
SCIENTIFIC CRIME DETECTION LABORATORY

DATE: 04/12/2004

TIME: 15:30

DIAGNOSTIC CHECK

COMPONENT: OKAY
PROGRAM: OKAY
SOFTWARE: OKAY
HEATER: OKAY
SAMPLE CHAMBER: YES
BREATH TUBE: YES
PUMP: OKAY
FLOW DETECTOR: OKAY
HIGH SPEED: OKAY
DISCOUR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTED TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
SCIENTIFIC CRIME DETECTION LABORATORY